




Data file: C:\CHEM32\1\DATA\210221\20210129 2021-02-21 08-50-44\602755
21010046Final HCl.D

Sample name: 602755 21010046Final HCl

Description: Mobile phase: Buffer A: 0.1%TFA in H2O
Buffer B: 0.1%TFA in ACN
Gradient: 26-36% B in 20min , Flow rate: 1.0ml/min
Column: phenomenex C18, 4.6*150mm, 5um 100A (A-0010)
Instrument: Agilent HPLC 1100

Instrument: 1100 Location: 46
Injection date: 2021/2/21 9:19:49 Injection: 1 of 1
Last changed: 2021/2/21 10:27:30 Injection volume: 2.000
Acq. operator:

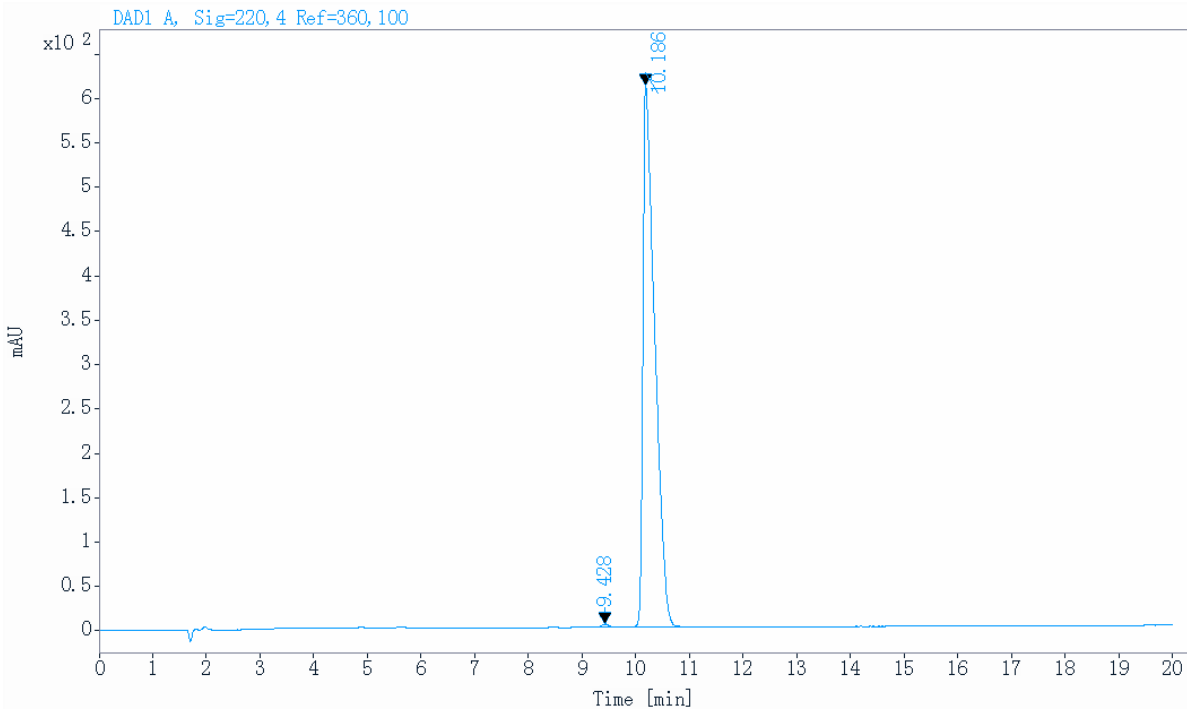

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area%	Name
9.428	BB	0.1544	38.3480	3.7155	0.4092	
10.186	BV R	0.2141	9332.3301	611.3965	99.5908	
	Sum		9370.6781			